HOFFRICHTER TECHNOLOGY FOR EASY BREATHING

01. Description

The ultrafilter is provided for filtering the therapy air of the respiratory therapy device **point®.** The ultrafilter is more efficient than the standard filter, because it is bigger and filters the respiratory therapy air twice. This filter may give relief to patients suffering from allergic reactions.

It comprises
1 the filter cartridge,
2 a coarse filter,
3 and an ultrafilter.

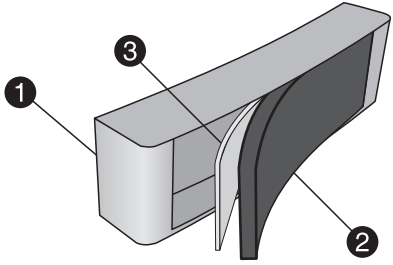

Clean the coarse filter once a week. To do this, remove the filter cartridge and take the coarse filter out of the cartridge. Wash out the coarse filter using mild soap water. Then thoroughly rinse with water. Before being re-inserted, the coarse filter must be completely dry.
The white double-layer ultrafilter cannot be cleaned. It should be visually checked once a week and must be exchanged once a month or, if it is very dirty, even more often. To exchange the ultrafilter, remove the filter cartridge and first take out the coarse filter. Then you can remove and exchange the ultrafilter.

Proceed as follows to attach the filter system:

a Remove the standard coarse filter.

b Fit on the filter cartridge 1.

c Ensure that you fit the filter system in the proper position. The cartridge must be positioned flush with the bottom side of the device.

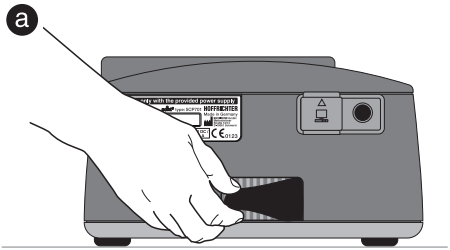

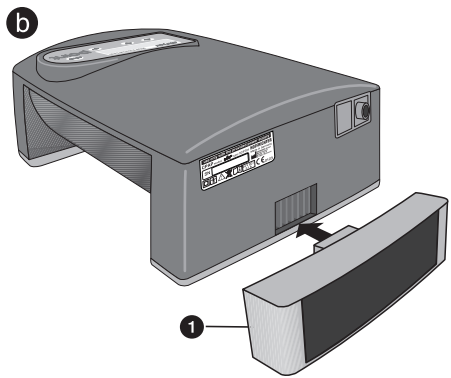

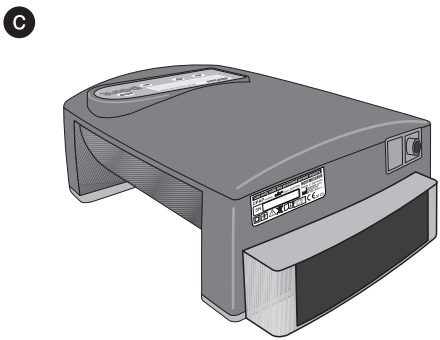

Manufacturer

HOFFRICHTER GmbH
Mettenheimer Strasse 12/14
D-19061 Schwerin
Germany

Phone: +49-385-39925-0
Fax: +49-385-39925-25
Mail to: info@hoffrichter.de
URL: www.hoffrichter.de

Dealer's stamp